


ELECTRICAL LAYOUT

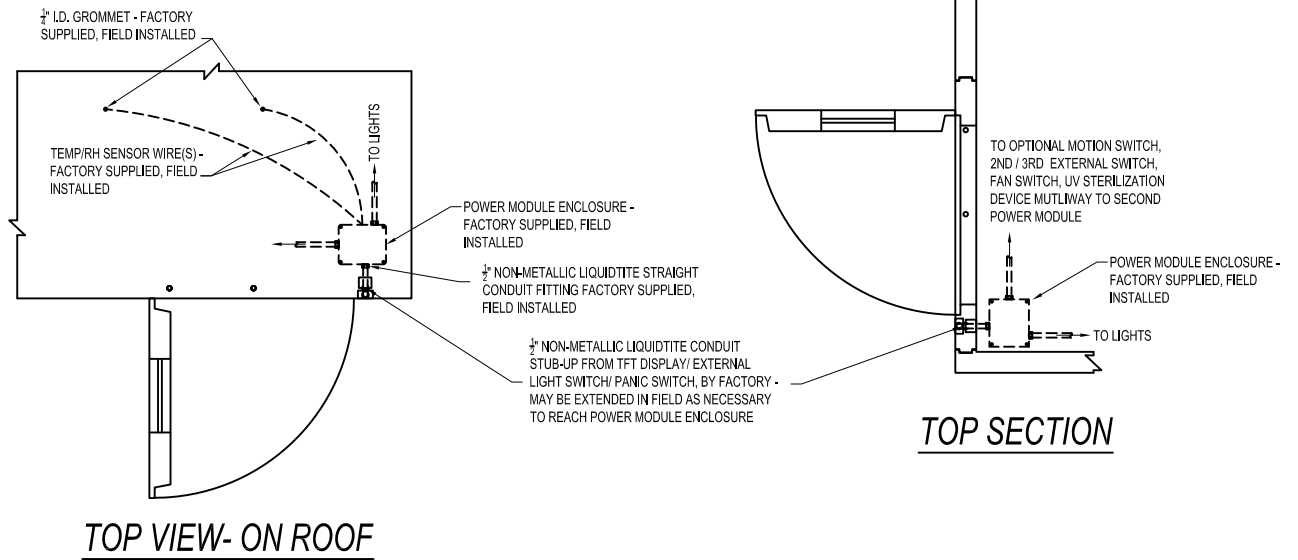

NOTE:
 ALL WIRES STUBBED UP FROM INTERIOR OF ROOM FOR CONNECTION TO POWER MODULE MUST BE TAGGED AND LABELED FOR FIELD CONNECTION PER THE FOLLOWING CONVENTION (REFERENCE SMARTRITE 100 WIRING DIAGRAM SMRT100WD):

STUB-UP WIRE TAGS		
TAG	DEVICE NAME	CABLE/WIRE TYPE
ELS	EXTERNAL LIGHT SWITCH	LOW VOLTAGE
PS	PANIC SWITCH	LOW VOLTAGE
DS#_	DOOR SWITCH #1, #2	LOW VOLTAGE
MD	MOTION DETECTOR	LOW VOLTAGE
TFT	SMRT-100 TFT DISPLAY	LOW VOLTAGE
DH#_	DOOR JAMB HEATER #1, #2	#14-16 AWG - BK, W, G
VP	HEATED VU PORT	#14-16 AWG - BK, W, G
UV	UV STERILIZATION RECEPTACLE	#14-16 AWG - BK, W, G
LGT	JAMB LIGHT	#14-16 AWG - BK, W, G

REVISIONS			
NO.	DATE	BY	DESCRIPTION

THIS DRAWING IS THE PROPERTY OF EVERIDGE. IT IS NOT TO BE ALTERED OR DISTRIBUTED TO OTHERS WITHOUT THE WRITTEN APPROVAL OF EVERIDGE.



SMARTRITE OEM MANUFACTURING
 DETAILS

05 MAY 2023 SC DWG# SMRT100MFG